


Sample Name	CS014415	Position	P1-C9	Instrument Name	Instrument 1	User Name	
Inj Vol	Unknown / Injection	InjPosition		SampleType	Sample	IRM Calibration Status	Success
Data Filename	CS014415.d	ACQ Method	0923-1-neg.m	Comment		Acquired Time	10/10/2021 8:53:43 PM

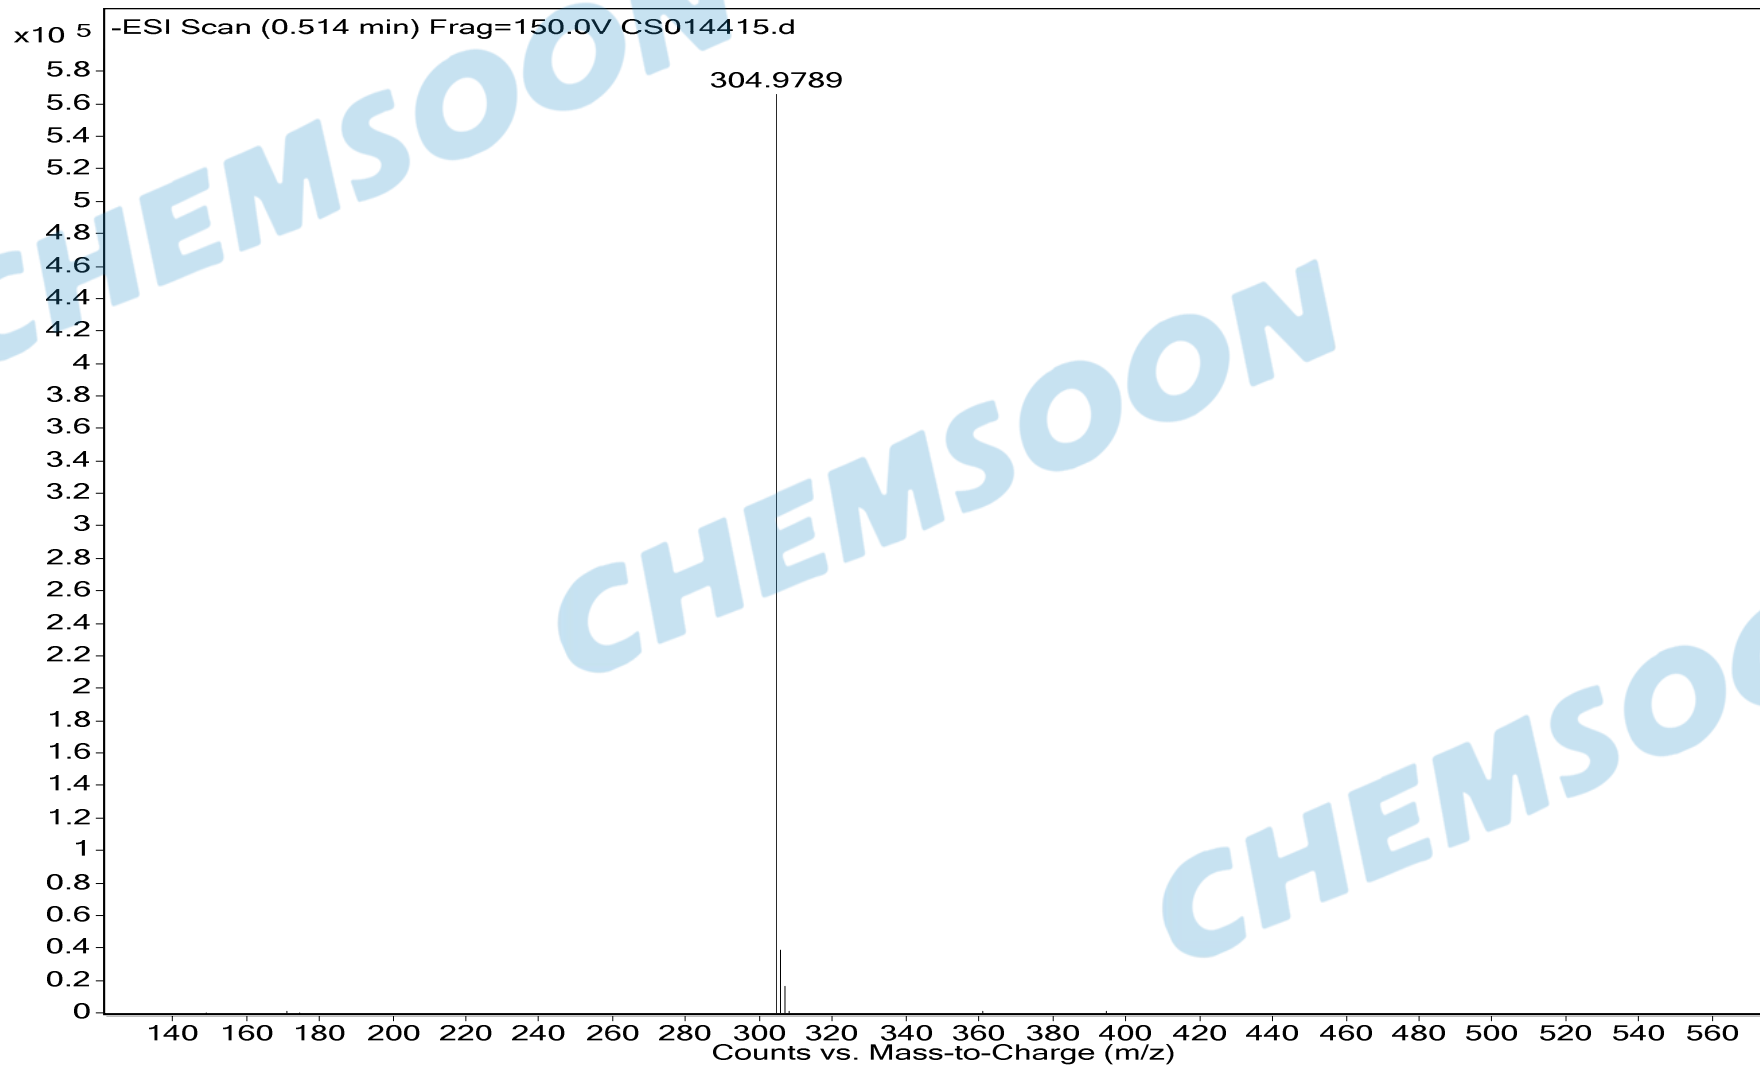

**CHEMSOON**

**CHEMSOON**

**CHEMSOON**